


Tue Sep 26 12:14:34 2006


TIDE Mass_1

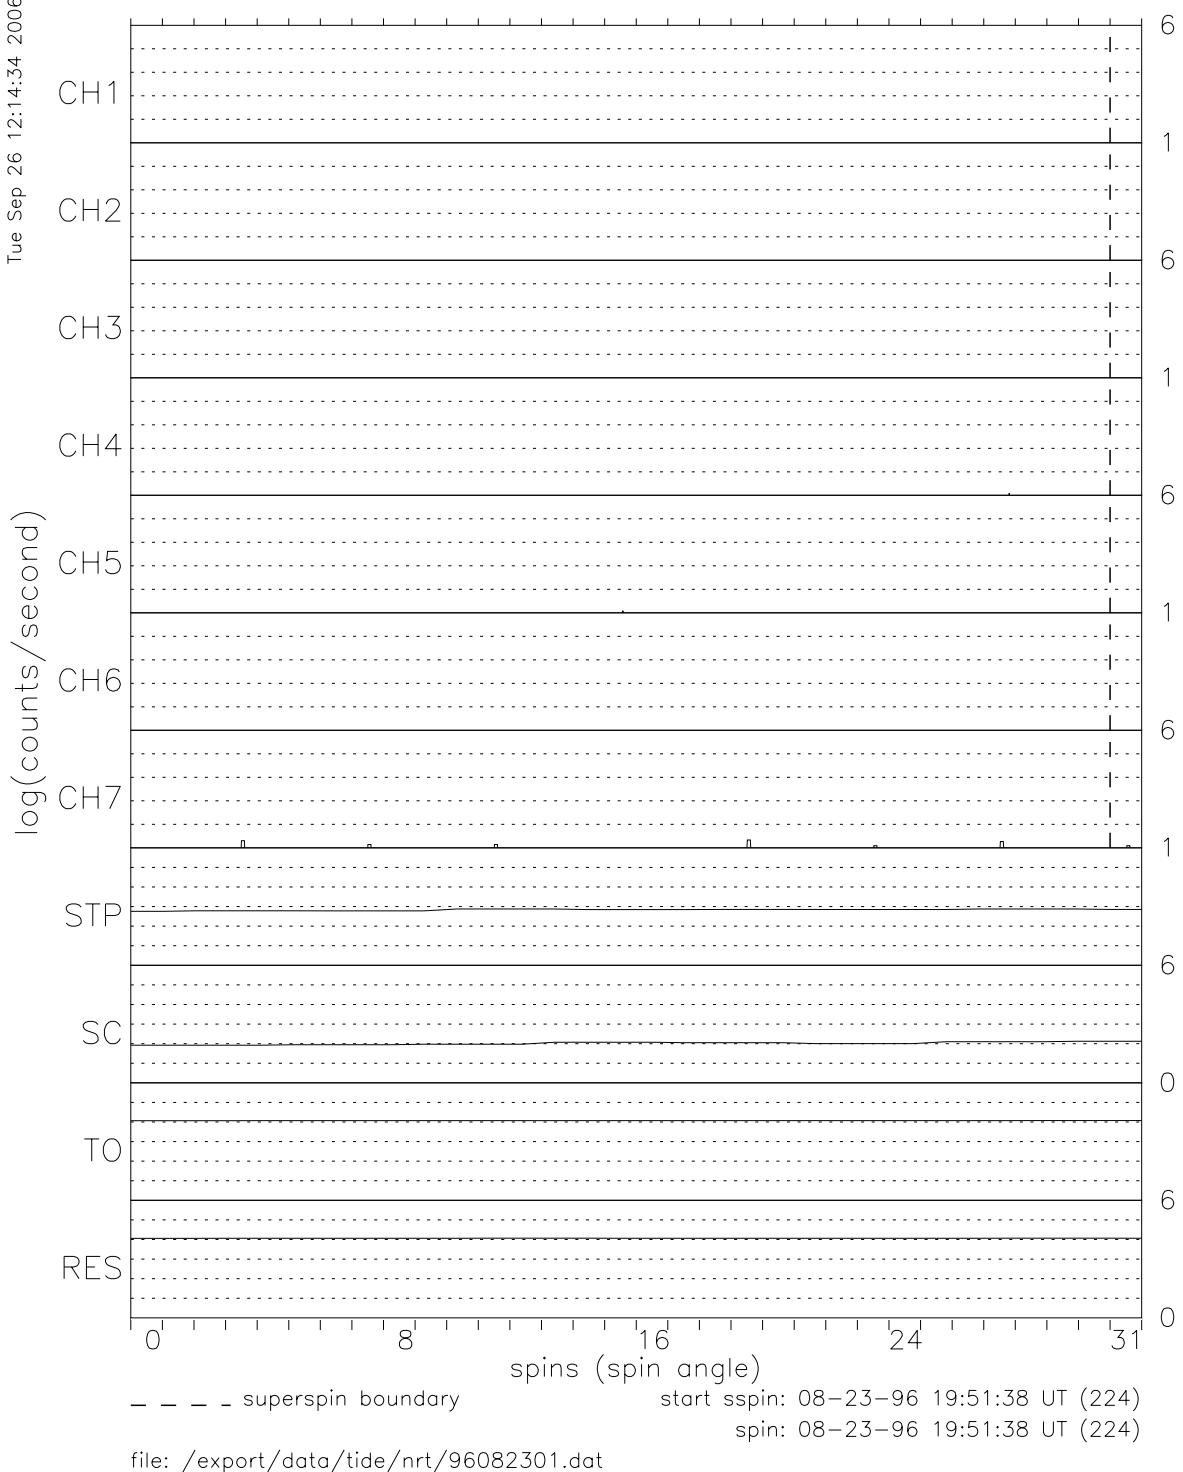

-15kV TOF: -9051 v
-3.6kV MCP: -2688 v
-2.4kV MCP: -1640 v
Input Cur: 292 ma
RPA max: 236 v
Mirror max: 238 v

Tue Sep 26 12:14:34 2006

TIDE Direct Events

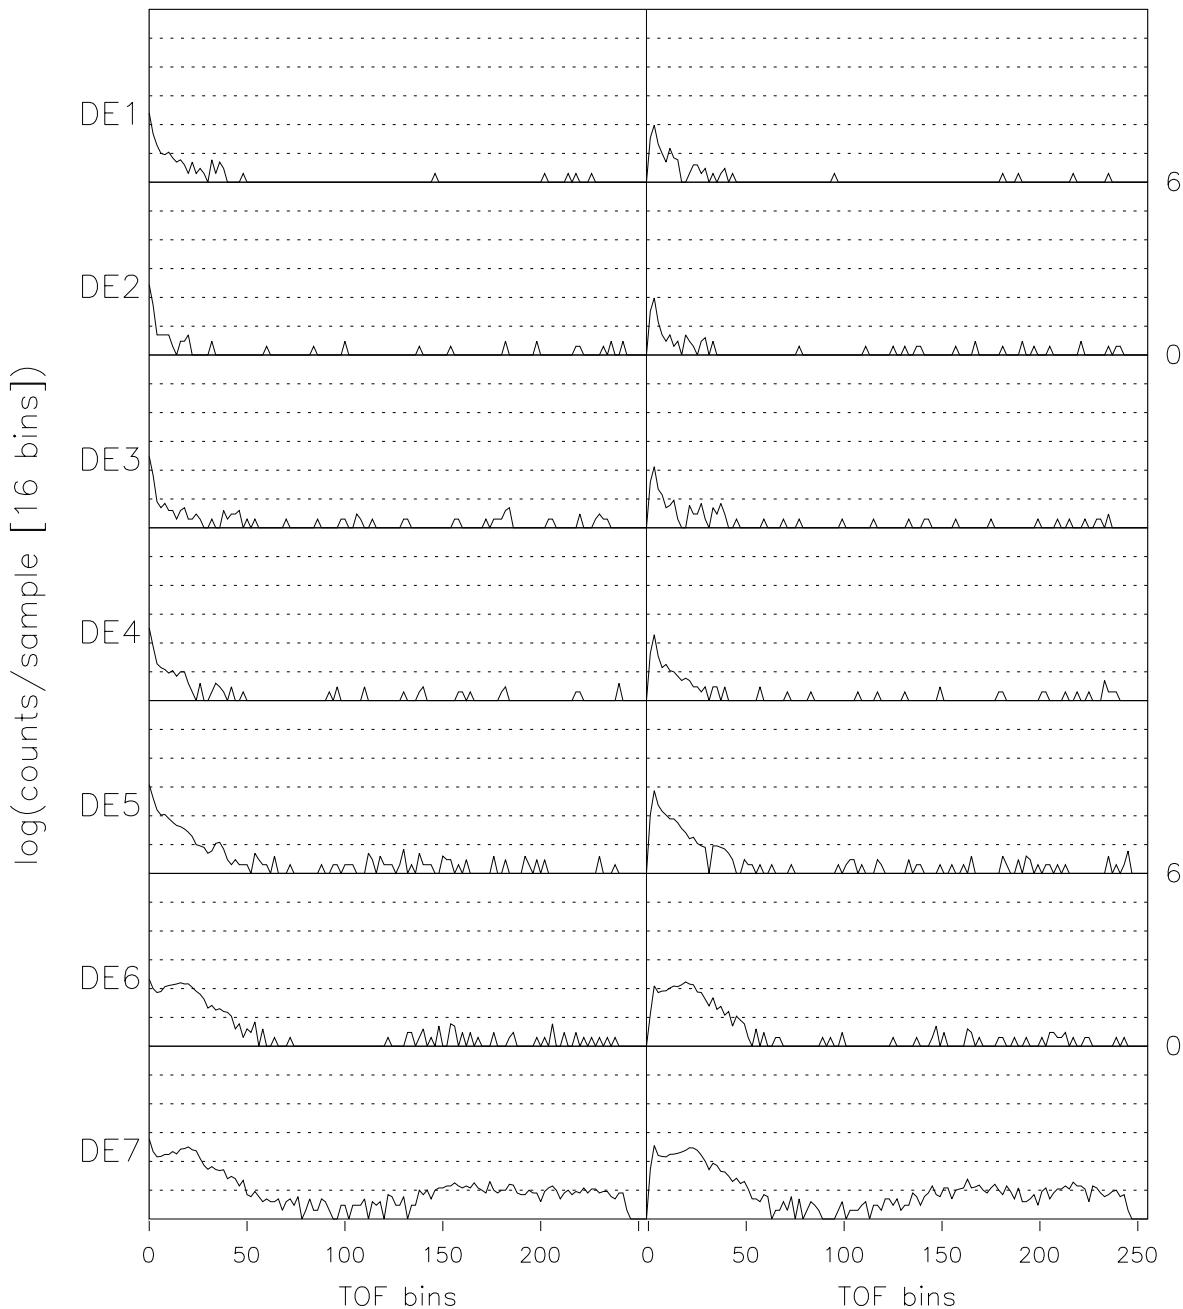

reported: 08-23-96 19:45:11 UT

reported: 08-23-96 19:48:21 UT

file: /export/data/tide/nrt/96082301.dat

-15kV TOF: -9051 v

-3.6kV MCP: -2672 v

-2.4kV MCP: -1610 v

Input Cur: 302 ma

RPA max: 236 v

Mirror max: 238 v